

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Heart's Desire Farm, LLC/Mike Harnett
Rt 2, Box 750
Shinnston WV 26431 USA

04/13/10

Test No: 372533


Animal and Sample Description

Animal Name: HDF Paisley
Breed: Alpaca(Huacaya)
Sex: Female
Color: Medium Fawn

Animal ID: XXXXX
Sample Location: Side
Sample Date: 03/31/10
Age: 08/08/09

Laboratory Data

Mean Fiber Diameter: 17.9 microns
Standard Deviation: 3.8 microns
Coefficient of Variation: 21.4 %
Fibers Greater Than 30 microns: 1.0 %

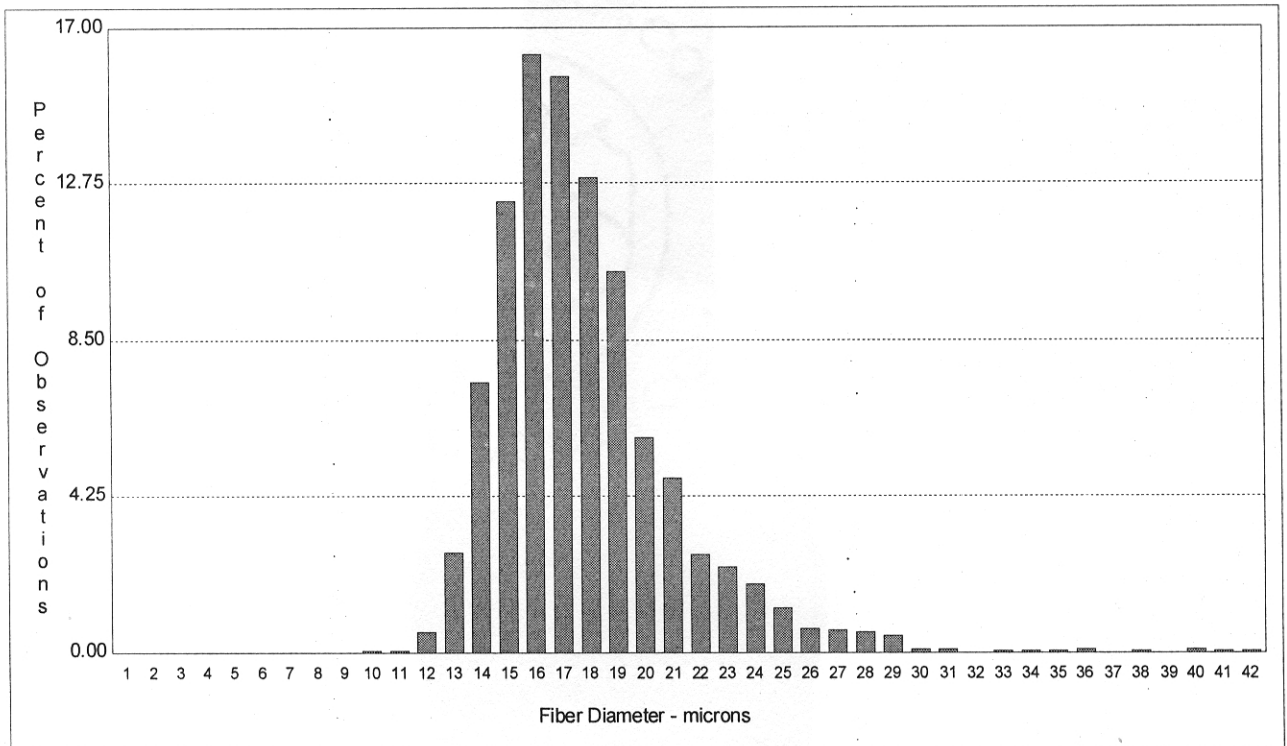

This Test Performed According to I.W.T.O Method 12