



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Shambalah Alpaca Ranch/Hillary J Devin  
7157 E Park Dr  
Franktown CO 80116-9631

**Date:** 08/09/19  
**Shear ID:** 187296  
**Test No:** 979291


### Animal and Sample Description

**Animal Name:** Kiva's Fallon  
**ARI #:** 310040075  
**Breed:** Alpaca(Suri)  
**Sex:** Female  
**Color:** Med Fawn

**Date of Birth (Age):** 09/22/08  
**Sample Location:** Side  
**Sample Date:** 06/01/19  
**Previous Shear Date:** 06/02/18  
**Total Fleece Wt (lbs):** 3.00

### Laboratory Data

<b>Mean Fiber Diameter:</b>	30.9 microns	<b>Mean Staple Length:</b>	112.0 mm
<b>Standard Deviation:</b>	7.0 microns	<b>Length Standard Deviation:</b>	2.1 mm
<b>Coefficient of Variation:</b>	22.7 %	<b>Length Coefficient of Variation:</b>	1.9 %
<b>Spin Fineness:</b>	30.5 microns	<b>Mean Curvature:</b>	8.0 deg/mm
<b>Fibers Greater Than 30 microns:</b>	41.8 %	<b>SD Curvature:</b>	8.8 deg/mm
<b>Comfort Factor:</b>	58.2 %		

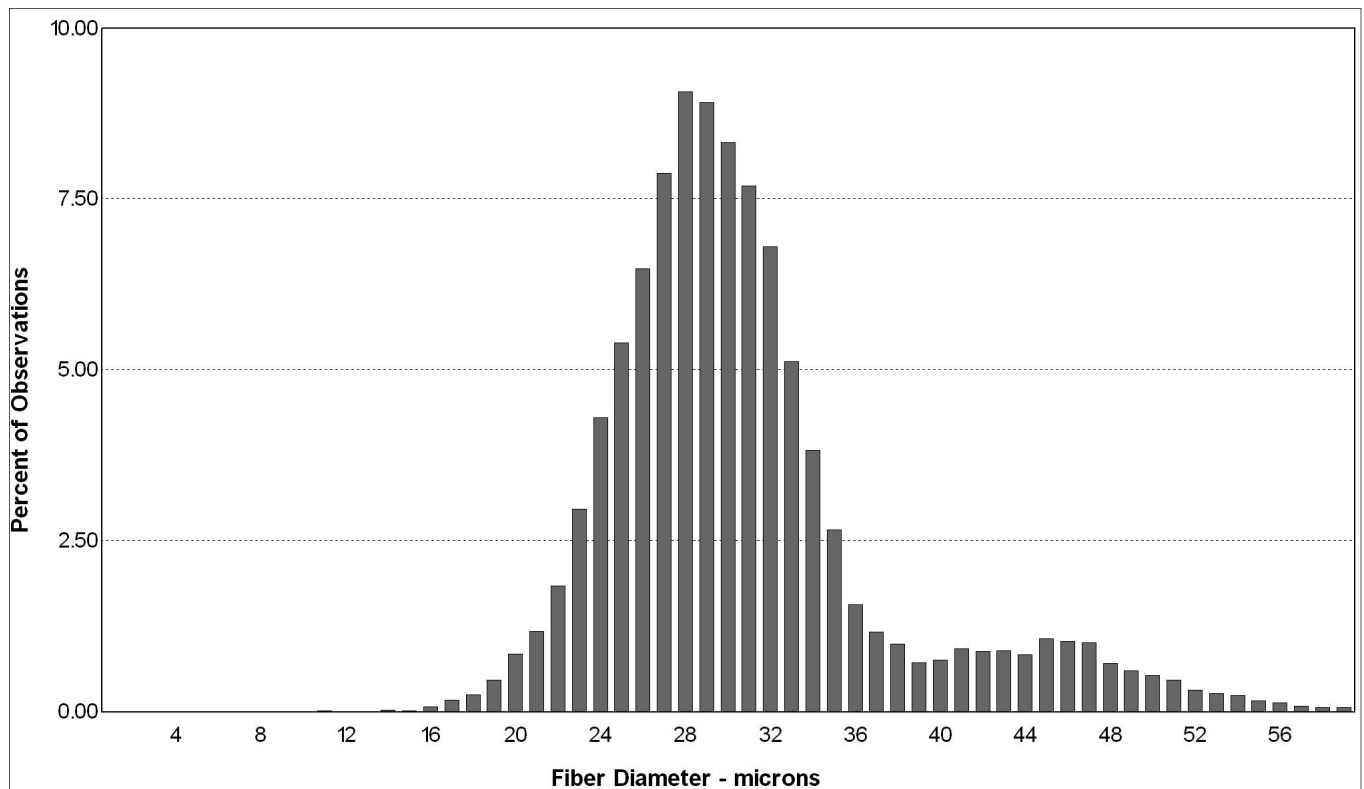

This Test Performed According to I.W.T.O Method 47